

FIG. 3

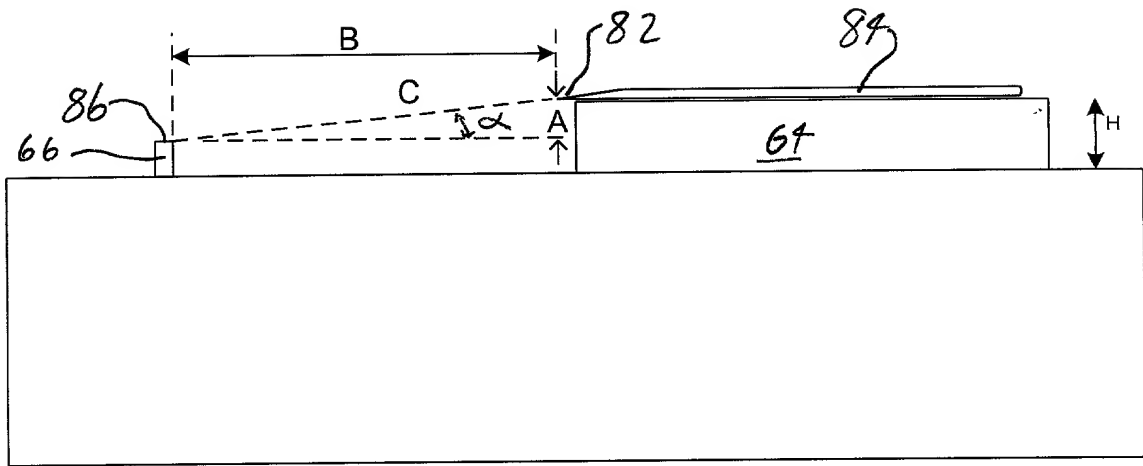


FIG. 4

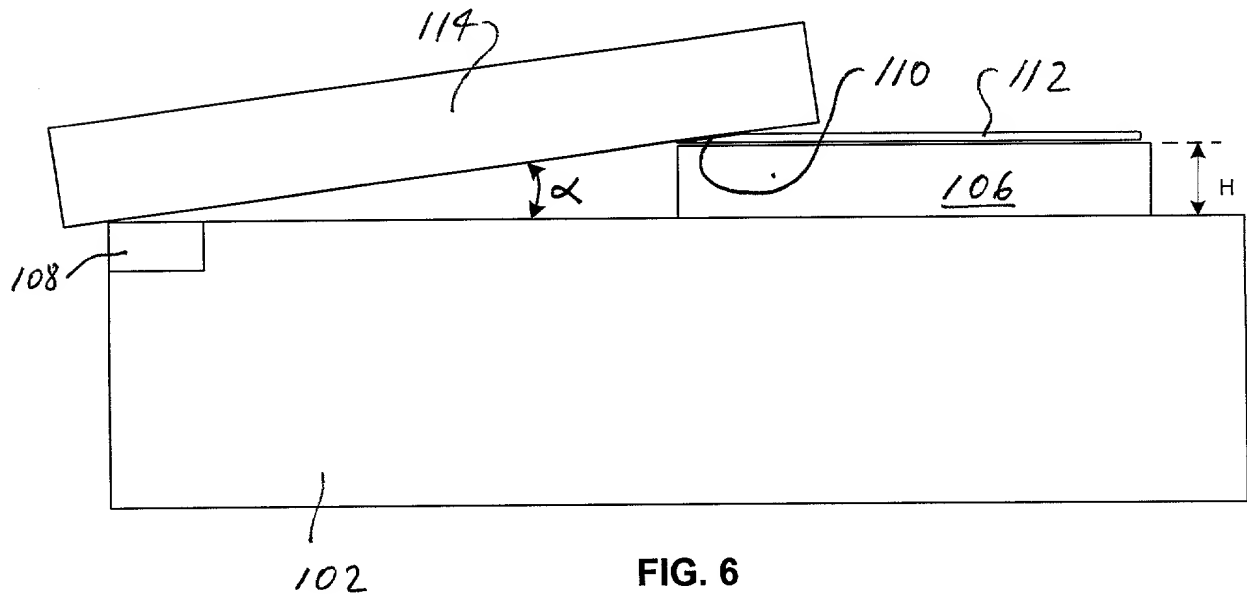


FIG. 6

FIG. 5 is a cross-sectional view of the device 100.

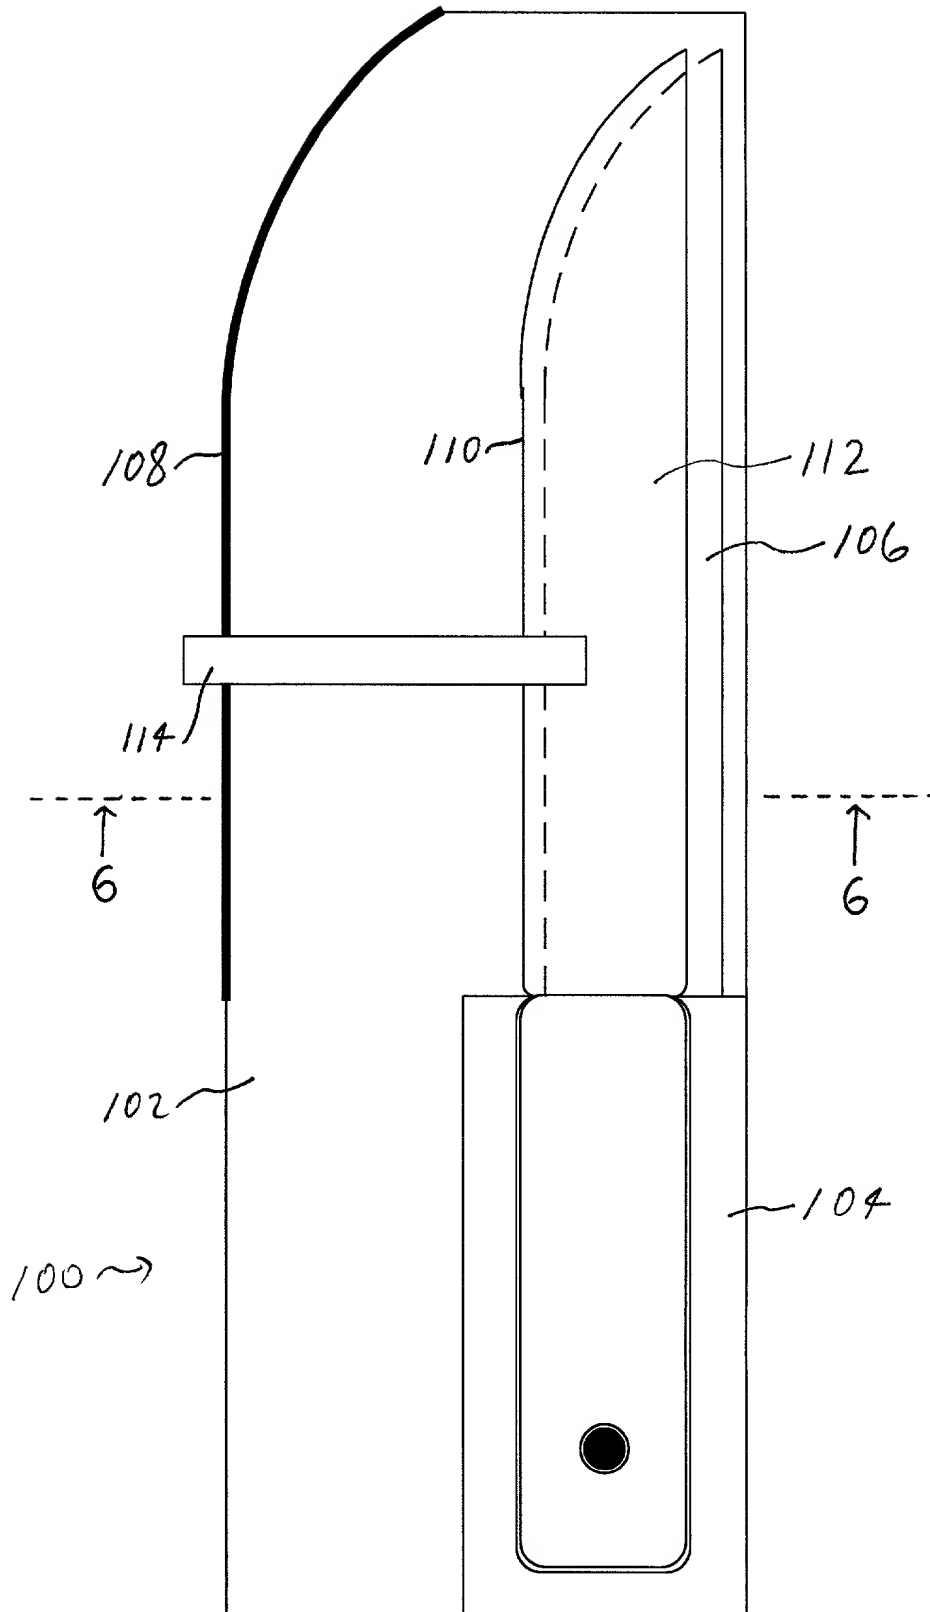


FIG. 5

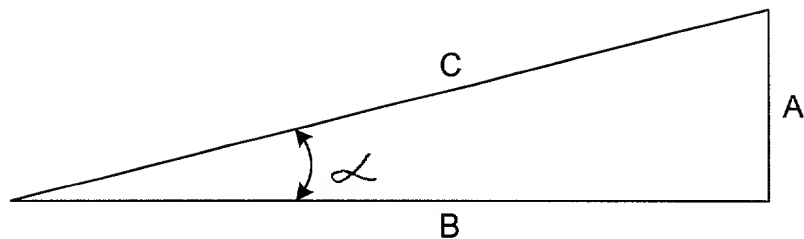


FIG. 7

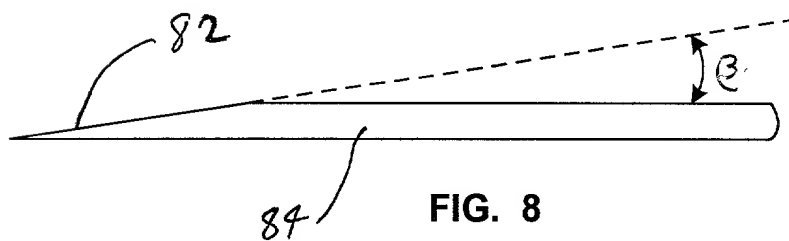


FIG. 8